

## Transaction Information

Tool ID	MSCD703
Tool Status	Connected
Location	Woodlands, Singapore
Wafer Size	300 mm
Fab Section	Metrology
Tool Available Date	2024-08-02

## General Product Information

Vendor Supplier	KLA-TENCOR
Model	SPECTRACD-XT
Vintage	2009
Serial No	6511267
Asset Description	OCD Measurement Tool
Software Version	050032
CIM	SECS/GEM
Process	OCD Measurement

## Hardware Configuration (Fab)

System Type	Description	Quantity	Status
Main System	MainFrame	1	OK
Others			

## Hardware Configuration (Subfab / Auxilliary Units)

Description	Quantity	Status
NONE		


## Missing/Faulty Parts / Accesories List

Description	Quantity
NONE	

# Tool Pictures

General

MainFrame

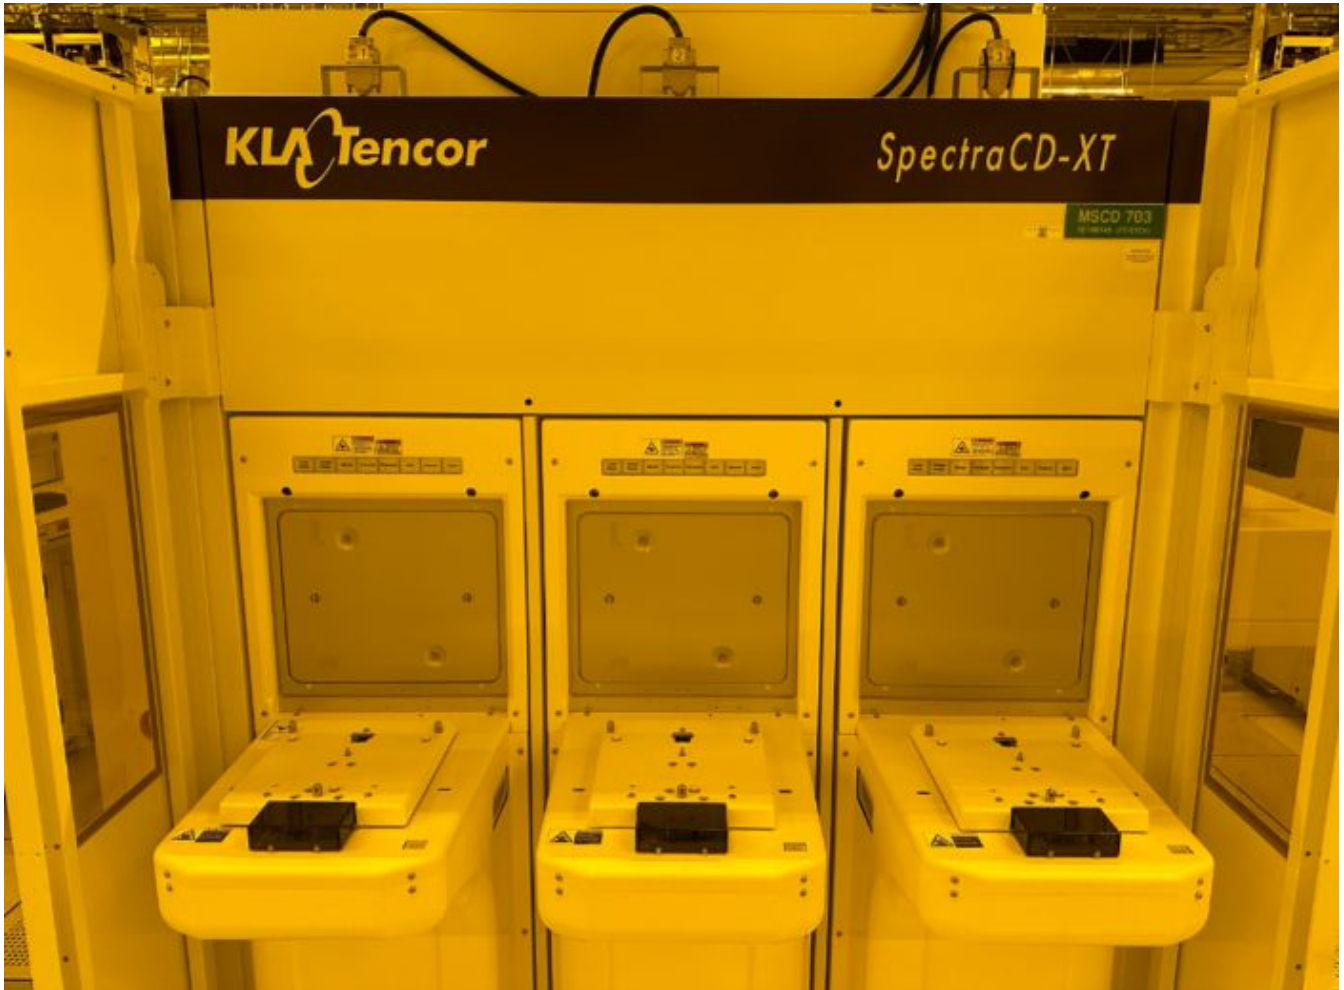

Hardware Fab

Handler



Manufacture Serial

SN

**KLA Tencor**

**SERVICE PERSONNEL ONLY**

Haticshoret St. Migdal Ha'Emek 23100 ISRAEL

MODEL : ARCHER **CD-XT**

Mfg-Date: **02-FEB-2009**

SERIAL NO: **6511267**

V: **230 VAC**  
**208 VAC**

I: **11.3 A (230V)**  
**12.5 A (208V)**

f: **50/60 Hz**

Ph: **1  $\phi$  (230V)**  
**2  $\phi$  (208V)**

Main breaker rating: 13Amp  
Largest load rating: 5Amp  
Ampere Interrupt Capacity: 10,000Amp  
SCCR : 6,000 Amp  
Wiring configuration: 2 wire + Ground  
Diagram Number: **0215874-000**

THIS PRODUCT IS PROTECTED BY  
U.S. PATENTS 4,818,110 & 5,112,129  
& 5,438,413

OTHER PATENTS PENDING  
MADE IN ISRAEL

**TAGOUT/LOCKOUT PROCEDURE**

1. Power the system down.
2. Place the Main circuit breaker on the OFF position.
3. Insert the locking device "ears" in the holes on the circuit breaker body above the ON/OFF lever by pulling the yellow cover to allow free motion of the metal "ears".
4. Push the yellow plastic cover back into place.
5. Place the lock provided in the kit on the opening of the locking device.

## Additional Tool Data Files